


DMM7512 Dual Channel 7½-Digit Sampling Multimeter

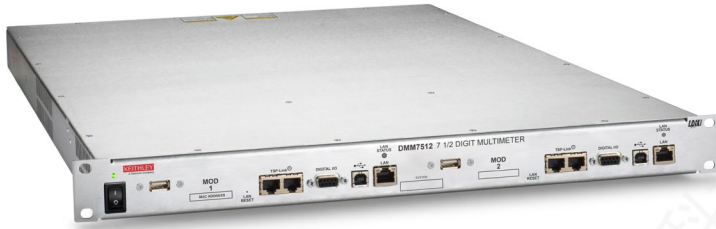

KEITHLEY
A Tektronix Company

Key Features

- Two high-precision, 7½-digit DMMs in a 1U high, full rack width chassis
- No space requirements between instruments minimizes rack space
- Capture waveforms or identify transients with two 1 Msample/s 18-bit digitizers
- Trigger a waveform measurement on a signal level, a rising or falling edge, a window, or a digital trigger
- Store up to 27.5M timestamped readings on a waveform
- Basic one-year DC Voltage accuracy as low as 14 ppm
- 10 nV, 0.1 $\mu\Omega$, and 1 pA sensitivities for making high resolution low level measurements such as measurements of portable device sleep currents
- High accuracy, low resistance measurements with offset compensated ohms, four-wire measurement, and dry circuit functions
- Auto-calibration improves accuracy and stability by minimizing temperature and time drift
- USBTMC-compliant and LAN LXI-compliant interfaces
- Reduce test time by executing test scripts with the Embedded Test Script Processor, which saves PC command communication overhead
- Tight synchronization between the two DMMs using TSP-Link® communication
- Reduce life cycle costs with a two-year calibration interval

The DMM7512 Dual Channel 7½-digit Sampling Multimeter combines two full-function, high accuracy and high sampling speed DMMs into a compact 1U high, full rack wide form factor chassis. The compact chassis saves rack space in high-instrument density, test systems. The small size does not compromise measurement performance. Each DMM has identical functionality, and both are entirely independent of each other. The DMMs achieve a basic, one-year accuracy as low as 14 ppm for DC volts, 24 ppm for resistance, and 60 ppm for DC current. Sensitivities of 10 nV, 0.1 $\mu\Omega$, and 1 pA ensure high quality, high resolution measurements on very small signals. In addition, each DMM has a wide range of functionality including voltage digitizing, current digitizing, and temperature measurements with resistance temperature detectors (RTDs), thermistors, and thermocouples. With dual channel capability, fast signal sampling, high speed data transfer rates reaching up to 100,000 measurements/s, and internal execution of program test scripts, the DMM7512 reduces space and reduces test time in automated test systems.

Capture Low Level Waveforms with the 1 Msample/s Digitizer

Avoid the need for a separate instrument to capture waveform parameters or ensure a waveform is within design limits by using the digitizing function. Digitize either voltage or current and sample a waveform at a rate of up to 1 Msamples/s with the 18-bit digitizer. The digitizing function employs the same ranges that the DC voltage and DC current functions use to deliver exceptional dynamic measurement range. With the digitizer's 1 μV and 0.1 nA sensitivities, the DMM7512 is the best solution for measuring low level waveforms such as wireless IoT battery current profiles and laser diode current consumption profiles. Using the digitizing function, the two DMMs can measure the current in all the operating states of a device including the sleep state and the current burst state when the device is transmitting. By using the two DMMs as synchronized digitizers, one for voltage and one for current, power can be accurately computed on time-varying waveforms.

日图简介

深圳市日图科技有限公司（简称“日图科技”）创始于2004年，核心业务是为国内企业提供测试设备及相关器材的供应服务，公司客户涵盖制造、科研、教育、电力、能源、通信等众多领域。创业至今，日图科技已经成为国内仪器仪表行业中最大的综合服务供应商之一，日图科技作为行内的领先者，有着高效的供应服务体系，并拥有一支专业的、高素质的服务团队。

目前，日图科技已在深圳、上海、广州、苏州、重庆、杭州、西安、香港等国内电子工业发达地区设立了办事与服务机构，并通过日图科技在全国各地的经销网络，为广大客户提供优质的本地化服务。


日图科技一贯秉承“专业、规范，诚信立业，日日图新”的宗旨，并在实践中不断提升公司的服务能力，为客户提供专业、高效、全面、经济的优质供应服务，顾客满意是日图科技永远追求的目标。

合作伙伴




优势服务


- (1) 产品选型
- (2) 测试解决方案
- (3) 免费测试服务
- (4) 代办计量校准
- (5) 维修维护
- (6) 技术培训
- (7) 物流配送
- (8) 常备应急库存

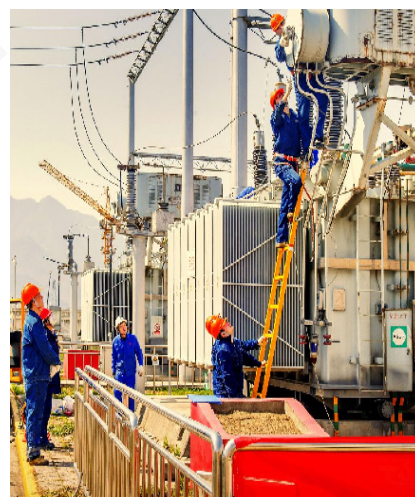

DMM7512 Front Panel Shows the two DMM's multiple, communication interfaces.

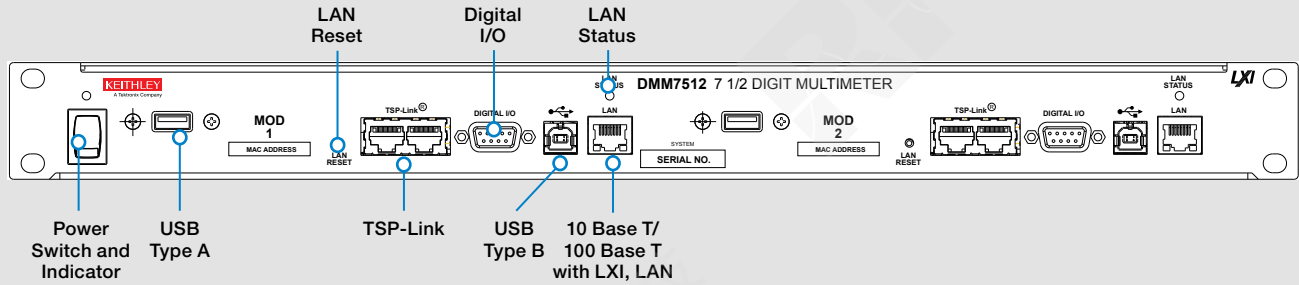

DMM7512 Rear Panel Shows the identical measurement inputs for DMM 1 and DMM 2.

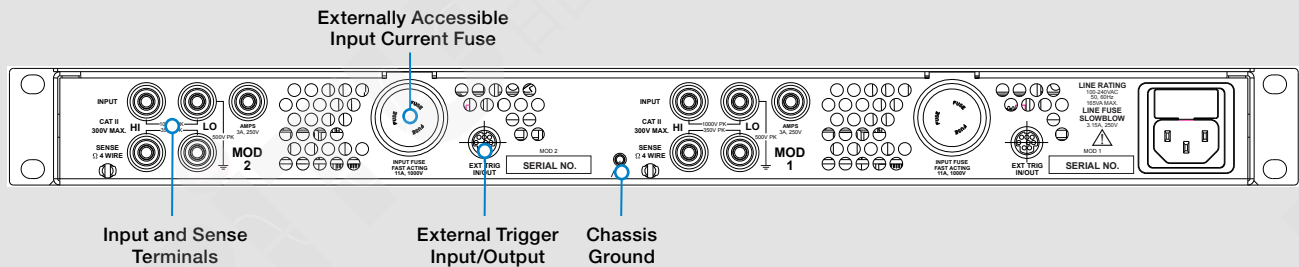

The digitizers can trigger on either the slope, a level, or a window of an input waveform. The digitizers can also trigger on digital control signals such as external, hardware trigger inputs and software trigger commands. Each digitizer function provides oscilloscope-like performance with excellent sensitivity, high resolution, and a fast sampling rate.


Optimized to Maximize Throughput

In addition to the high-speed sampling and fast integrating measurement modes, each of the DMM7512's DMMs utilize Keithley's powerful Test Script Processor (TSP®) technology. This embedded scripting capability enables each DMM to run powerful test scripts directly on the instrument without external PC interaction. These test scripts are complete test programs based on an easy-to-use, yet highly efficient and compact scripting language, Lua (www.lua.org). Scripts include instrument control commands and program statements. Program statements control script execution and include typical programming language features such as variables, functions, branching, and loop control. A test script can execute a complete


test including performing specialized computations and making decisions on results without having to receive and decode individual commands from a controller. This saves significant test time by eliminating a substantial amount of interface communication time.

TSP technology also offers instrument-to-instrument communication and control through the TSP-Link® channel expansion bus. The DMMs in the DMM7512 can communicate with each other and with other TSP-enabled instruments, such as the 4-channel 2606B System SourceMeter® Source Measure Unit (SMU) Instrument, in a master-subordinate configuration so that all instruments operate as a single, integrated system controlled by a TSP script in the master instrument. TSP-Link supports up to 32 instruments per IP address, so a system can be easily scaled for any test system requirements.

In addition to communicating with and controlling TSP-enabled instruments, any instrument with a LAN interface can be controlled by a TSP-embedded test script using the TSP-Net communication facility.

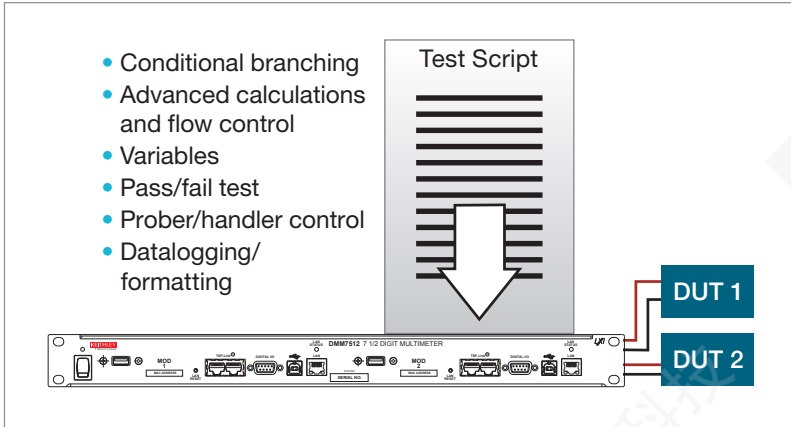

Embedded TSP test scripts execute complete test programs and reduce test time.

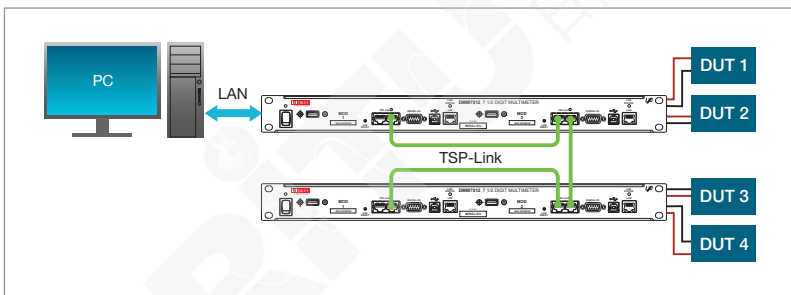

A test script can control multiple instruments through the TSP-Link interface. Measurements between all DMMs can be synchronized with a latency of under 500 ns.




Simultaneously stimulate and measure multiple DUTs with the compact, high density, configuration of the dual-DMM7512 and the four-channel 2606B System SourceMeter SMU Instrument.

Use the Virtual Front Panel for Test Setup or Manual Measurements

Even though the DMM7512 does not have a front panel display, the instrument has a built-in web browser with a virtual front panel. Through a LAN interface connection, the virtual front panel can be displayed on a PC monitor. With the virtual front panel, each DMM of the DMM7512 can be controlled using either the PC touchscreen display or mouse and keyboard controls. All the functionality of each DMM can be accessed through the virtual front panel. Thus manual operation and test setup can be performed as easily as if the instrument had a physical front panel.



The DMM7512 virtual front panel displays a conventional DMM front panel.

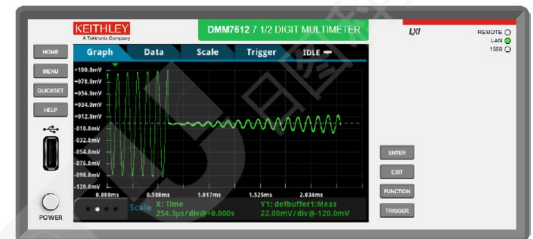

Use the virtual front panel to obtain a full screen display of a waveform. Apply cursors and statistics for waveform analysis.

Specification Conditions

This document contains specifications and supplemental information for the DMM7512 7½ Digit Graphical Sampling Multimeter instrument. Specifications are the standards against which the DMM7512 is tested. Upon leaving the factory, the DMM7512 meets these specifications. Supplemental and typical values are nonwarranted, apply at 23 °C, and are provided solely as useful information. Measurement accuracies are specified at the DMM7512 terminals under these conditions:

- Temperature 23 °C ±5 °C, 5% to 80 60% relative humidity, noncondensing
- After a 4-hour warmup period
- 1 PLC or 5 PLC; for NPLC settings less than 1 PLC, add appropriate ppm of range for peak noise uncertainty from the RMS noise table
- Autozero enabled unless otherwise noted
- Remote sense operation or properly zeroed local operation
- Calibration period: One year or two years (calibration period may vary depending on customer requirements)
- T_{ACAL} = Ambient temperature of last automatic calibration
- T_{CAL} = Ambient temperature of last external calibration; factory calibration performed at 23 °C ±1 °C

DC Voltage

Accuracy (Input impedance auto)

| Range ¹ | Resolution | Input Impedance | Accuracy ±(ppm of reading + ppm of range) | | | | |
|----------------------------|------------|-------------------------|--|---|---|---|--------------------------------------|
| | | | 24 hour $T_{CAL} \pm 1 \text{ } ^\circ\text{C}^2$ | 90 day $T_{CAL} \pm 5 \text{ } ^\circ\text{C}$ | 1 year $T_{CAL} \pm 5 \text{ } ^\circ\text{C}$ | 2 year $T_{CAL} \pm 5 \text{ } ^\circ\text{C}$ | Temperature Coefficient ³ |
| 100.00000 mV ⁴ | 10 nV | > 10 GΩ or 10 MΩ ±1% | 6 + 30 | 12 + 30 | 18 + 30 | 29 + 30 | 0.1 + 2.5 |
| 1.0000000 V ⁴ | 100 nV | > 10 GΩ or 10 MΩ ±1% | 4 + 2 | 9 + 5 | 15 + 5 | 26 + 5 | 0.1 + 0.5 |
| 10.000000 V ⁴ | 1 μV | > 10 GΩ or 10 MΩ ±1% | 2 + 0.7 | 9 + 1.2 | 14 + 1.2 | 22 + 1.2 | 0.1 + 0.05 |
| 100.00000 V ⁴ | 10 μV | 10 MΩ ±1% | 8 + 6 | (18 + 15) ⁵ | (22 + 15) ⁵ | (30 + 15) ⁵ | (0.15 + 0.1) ⁵ |
| | | | | 35 + 15 | 40 + 15 | 45 + 15 | 2.0 + 1 |
| 1000.0000 V ^{4,6} | 100 μV | 10 MΩ ±1% | 8 + 6 | (19 + 10) ⁵ | (23 + 10) ⁵ | (31 + 10) ⁵ | (0.15 + 0.1) ⁵ |
| | | | | 35 + 10 | 40 + 10 | 45 + 8 | 2.0 + 1 |

NOTES

1. 20% overrange on all ranges except 1% for 1000 V range.
2. Relative to calibration accuracy.
3. Add per degree from $T_{CAL} \pm 5 \text{ } ^\circ\text{C}$.
4. When properly zeroed using the Rel function with external cables.
5. Specified within 30 days of autocalibration, $T_{OPER} \pm 5 \text{ } ^\circ\text{C}$ from T_{ACAL} .
6. For signal levels greater than 500 V, add 0.02 ppm/V to the ppm of the readings specification for measurements exceeding 500 V.

RMS NOISE (ADDITIONAL PEAK NOISE UNCERTAINTY)⁷

Applies to ±ppm of range.

Peak noise uncertainty is included in DC specifications for ≥1 PLC.

Add peak noise uncertainty to measurements for <1 PLC.

Input impedance set to auto.

Examples

10 V at 0.006 PLC: 1.2 (from Accuracy table) + 11 (additional peak noise uncertainty) = 12.2 ppm of range.

10 V at 1 PLC: 1.2 + 0 = 1.2 ppm of range.

| NPLC | Digits | 100 mV | 1 V | 10 V | 100 V | 1000 V |
|------------------|--------|----------|-----------|-----------|-----------|-----------|
| 5 | 7½ | 0.5 | 0.08 | 0.06 | 0.3 | 0.06 |
| 1 | 7½ | 0.5 | 0.09 | 0.07 | 0.4 | 0.07 |
| 0.2 ⁸ | 6½ | 2 (10) | 0.2 (1.6) | 0.1 (1.1) | 1.1 (9.4) | 0.1 (1) |
| 0.2 | 6½ | 2 (12) | 0.2 (1.6) | 0.1 (1) | 1.1 (8.9) | 0.2 (1.1) |
| 0.06 | 5½ | 3 (17) | 0.4 (2.7) | 0.3 (2.1) | 3 (17) | 0.3 (2.4) |
| 0.006 | 4½ | 19 (95) | 3 (18) | 3 (15) | 34 (125) | 3 (18) |
| 0.0005 | 3½ | 95 (480) | 48 (215) | 36 (170) | 173 (800) | 40 (205) |

DC Voltage Characteristics

ADC Linearity

1.0 ppm of reading + 1.0 ppm of range

Input Impedance

100 mV to 10 V Ranges: Selectable >10 GΩ || <400 pF (auto) or 10 MΩ ±1% (10 MΩ)
100 V to 1000 V Ranges: 10 MΩ ±1%

Input Bias Current

<50 pA at 23 °C under the following conditions: Autozero off or input impedance 10 MΩ

Common Mode Current

<2.1 μA peak-peak in 1 MHz bandwidth
 <100 nA peak-peak in 1 kHz bandwidth

Common Mode Voltage

500 V_{PEAK} LO terminal to chassis maximum

DC Voltage Autozero Off Error

For ±1 °C and ≤10 minutes, add ±(8 ppm of reading + 15 μV)

Normal Mode Rejection

For DC voltage, line frequency ±0.1%

| | 5 PLC | 1 PLC | ≤0.2 PLC | ≤0.01 PLC |
|---------------|--------|-------|----------|-----------|
| Line Sync On | 110 dB | 90 dB | 45 dB | — |
| Line Sync Off | 60 dB | 60 dB | — | — |

Common Mode Rejection

For DC voltage and 100 Ω unbalanced in LO terminal

| NPLC | 5 | 1 | 0.2 | ≤ 0.2 |
|-----------|--------|--------|--------|-------|
| Line Sync | On | On | On | Off |
| CMRR | 140 dB | 140 dB | 120 dB | 80 dB |

NOTES

7. Noise values are based on 1000 readings with autozero on and using low thermal 4-wire short. VRMS noise is typical. Additional peak noise is guaranteed.

8. With line sync on.

Resistance

Enhanced Accuracy (within 30 days of autocalibration, $T_{OPER} \pm 5\text{ }^{\circ}\text{C}$ from T_{ACAL})⁹

| Range ¹⁰ | Resolution | Test Current ¹¹ ($\pm 5\%$) | Accuracy \pm [ppm of reading + ppm of range] | | | | |
|---|-----------------|---|--|---|---|---|--|
| | | | 24 Hour $T_{CAL} \pm 1\text{ }^{\circ}\text{C}$ ¹² | 90 Day $T_{CAL} \pm 5\text{ }^{\circ}\text{C}$ | 1 Year $T_{CAL} \pm 5\text{ }^{\circ}\text{C}$ | 2 Year $T_{CAL} \pm 5\text{ }^{\circ}\text{C}$ | Temperature Coefficient ¹³ |
| 1.0000000 Ω | 0.1 $\mu\Omega$ | 10 mA | 15 + 60 | 30 + 60 | 30 + 60 | 30 + 60 | 0.15 + 0.1 |
| 10.0000000 Ω | 1 $\mu\Omega$ | 10 mA | 15 + 6 | 30 + 6 | 30 + 6 | 30 + 6 | 0.15 + 0.1 |
| 100.000000 Ω | 10 $\mu\Omega$ | 1 mA | 12 + 4 | 27 + 4 | 27 + 4 | 27 + 4 | 0.15 + 0.1 |
| 1.00000000 k Ω | 100 $\mu\Omega$ | 1 mA | 12 + 3 | 24 + 3 | 24 + 3 | 24 + 3 | 0.15 + 0.1 |
| 10.0000000 k Ω ¹⁴ | 1 m Ω | 100 μA | 13 + 3 | 30 + 3 | 30 + 3 | 30 + 3 | 0.15 + 0.1 |
| 100.000000 k Ω ^{14, 15} | 10 m Ω | 10 μA | 13 + 3 | 30 + 3 | 30 + 3 | 30 + 3 | 0.3 + 0.1 |
| 1.00000000 M Ω ^{14, 16} | 100 m Ω | 10 μA | 14 + 3 | 30 + 4 | 30 + 4 | 30 + 4 | 0.7 + 0.1 |
| 10.0000000 M Ω ¹⁷ | 1 Ω | 0.69 μA 10 M Ω | 150 + 6 | 200 + 10 | 200 + 10 | 200 + 10 | 70 + 1 |
| 100.000000 M Ω ¹⁷ | 10 Ω | 0.69 μA 10 M Ω | 800 + 30 | 2000 + 30 | 2000 + 30 | 2000 + 30 | 385 + 1 |
| 1.00000000 G Ω ¹⁷ | 100 Ω | 0.69 μA 10 M Ω | 9000 + 100 | 9000 + 100 | 9000 + 100 | 9000 + 100 | 3000 + 1 |

Accuracy¹⁸

| Range ¹⁹ | Resolution | Test Current ²⁰ ($\pm 5\%$) | Accuracy \pm (ppm of reading + ppm of range) | | | | |
|----------------------------------|-----------------|---|--|---|---|---|--|
| | | | 24 Hour $T_{CAL} \pm 1\text{ }^{\circ}\text{C}$ ²¹ | 90 Day $T_{CAL} \pm 5\text{ }^{\circ}\text{C}$ | 1 Year $T_{CAL} \pm 5\text{ }^{\circ}\text{C}$ | 2 Year $T_{CAL} \pm 5\text{ }^{\circ}\text{C}$ | Temperature Coefficient ²² |
| 1 Ω | 0.1 $\mu\Omega$ | 10 mA | 15 + 60 | 40 + 60 | 50 + 60 | 70 + 60 | 2.5 + 5 |
| 10 Ω | 1 $\mu\Omega$ | 10 mA | 15 + 6 | 40 + 6 | 50 + 6 | 70 + 6 | 2.5 + 0.5 |
| 100 Ω | 10 $\mu\Omega$ | 1 mA | 12 + 4 | 35 + 4 | 47 + 4 | 65 + 4 | 5 + 0.25 |
| 1 k Ω | 100 $\mu\Omega$ | 1 mA | 12 + 3 | 30 + 3 | 41 + 3 | 65 + 3 | 5 + 0.25 |
| 10 k Ω ²³ | 1 m Ω | 100 μA | 10 + 3 | 30 + 3 | 42 + 3 | 65 + 3 | 2.5 + 0.25 |
| 100 k Ω ^{23, 24} | 10 m Ω | 10 μA | 13 + 3 | 38 + 3 | 50 + 3 | 65 + 3 | 5 + 1 |
| 1 M Ω ^{23, 25} | 100 m Ω | 10 μA | 14 + 3 | 38 + 5 | 50 + 5 | 65 + 5 | 5 + 1 |
| 10 M Ω ²⁶ | 1 Ω | 0.69 μA 10 M Ω | 150 + 6 | 200 + 10 | 400 + 10 | 600 + 12 | 70 + 1 |
| 100 M Ω ²⁶ | 10 Ω | 0.69 μA 10 M Ω | 800 + 30 | 2000 + 30 | 2000 + 30 | 2600 + 30 | 385 + 1 |
| 1 G Ω ²⁶ | 100 Ω | 0.69 μA 10 M Ω | 9000 + 200 | 9000 + 200 | 13000 + 200 | 14000 + 200 | 3000 + 1 |

NOTES

9. Specifications are for 4-wire resistance, offset compensation on for ≤ 10 k Ω measurements, and offset compensation off for ≥ 10 k Ω measurements. 1 Ω range is 4-wire only. For 2-wire, with Rel, add 50 m Ω to ppm of range uncertainty. Without Rel and with Model 1756 test leads, add 100 m Ω to ppm of range uncertainty.
10. 20% overrange on all ranges.
11. Test current with offset compensation off.
12. Relative to calibration accuracy.
13. Add per degree from $T_{CAL} \pm 5\text{ }^{\circ}\text{C}$.
14. Specifications are for external cable and load capacitance <1 nF.
15. For offset compensation on, add 10 ppm uncertainty to ppm of reading.
16. For 4-wire 1 M Ω , open lead detector on, add 10 ppm uncertainty to ppm of reading.
17. Specified for <10% lead resistance mismatch in HI and LO.
18. Specifications are for 4-wire resistance, offset compensation on for ≤ 10 k Ω measurements, and offset compensation off for ≥ 10 k Ω measurements. 1 Ω range is 4-wire only. For 2-wire, with Rel, add 50 m Ω to ppm of range uncertainty. Without Rel and with Model 1756 test leads, add 100 m Ω to ppm of range uncertainty.
19. 20% overrange on all ranges.
20. Test current with offset compensation off.
21. Relative to calibration accuracy.
22. Add per degree from $T_{CAL} \pm 5\text{ }^{\circ}\text{C}$.
23. Specifications are for external cable and load capacitance < 1 nF.
24. For offset compensation on, add 10 ppm of uncertainty to ppm of reading.
25. For 4-wire, 1 M Ω , open lead detection on, add 10 ppm uncertainty to ppm of reading.
26. Specified for <10% lead resistance mismatch in HI and LO.

Resistance Open Circuit DC Voltage²⁷

| Range ¹⁹ | 2-wire | Offset Compensation Off | Offset Compensation On |
|---------------------|--------|-------------------------|----------------------------|
| | | 4-wire | 4-wire |
| 1 Ω | – | 9.2 V | 9.5 V |
| 10 Ω | 9.2 V | 9.2 V | 9.5 V |
| 100 Ω, 1 kΩ | 14.0 V | 14.2 V | 14.3 V |
| 10 kΩ | 9.5 V | 9.5 V | 9.5 V |
| 100 kΩ, 1 MΩ | 12.7 V | 14.3 V | 14.3 V (100 kΩ range only) |
| 10 MΩ to 1 GΩ | 6.9 V | 6.9 V | – |

4-Wire Ohms (≤10kΩ) Offset Compensation On**RMS Noise (additional peak noise uncertainty)**²⁸

Applies to ± ppm of range.

Peak noise uncertainty is included in DC specifications for ≥1 PLC.

Add peak noise uncertainty to measurements for <1 PLC.

Examples

1 kΩ at 0.006 PLC: 3 (from Accuracy table) + 26 (additional peak noise uncertainty) = 29 ppm of range.

1 kΩ at 1 PLC: 3 + 0 = 3 ppm of range.

| NPLC | Digits | 1 Ω | 10 Ω | 100 Ω | 1 kΩ | 10 kΩ |
|-------------------|--------|-------------|-----------|-----------|-----------|-----------|
| 5 | 7½ | 2.8 | 0.3 | 0.3 | 0.07 | 0.3 |
| 1 | 7½ | 4.2 | 0.4 | 0.4 | 0.12 | 0.5 (2) |
| 0.2 ²⁹ | 6½ | 30 (160) | 3 (13) | 3 (13) | 0.4 (2.6) | 1.2 (8.2) |
| 0.2 | 6½ | 50 (250) | 5 (22) | 5 (22) | 0.6 (3.2) | 1.2 (8.3) |
| 0.06 | 5½ | 115 (546) | 11 (54) | 12 (56) | 1.1 (6.6) | 3 (18) |
| 0.006 | 4½ | 397 (2144) | 40 (215) | 38 (216) | 6 (34) | 15 (78) |
| 0.0005 | 3½ | 1767 (9333) | 177 (933) | 183 (954) | 85 (406) | 89 (456) |

2-Wire Ohms**RMS Noise (additional peak noise uncertainty)**²⁸

Applies to ± ppm of range.

Peak noise uncertainty is included in DC specifications for ≥1 PLC.

Add peak noise uncertainty to measurements for <1 PLC.

Examples

10 kΩ at 0.006 PLC: 3 (from Accuracy table) + 5 (50 mΩ with Rel) + 43 (additional peak noise uncertainty) = 51 ppm of range.

10 kΩ at 1 PLC: 3 + 5 + 0 = 8 ppm of range.

| NPLC | Digits | 10 Ω | 100 Ω | 1 kΩ | 10 kΩ |
|-------------------|--------|-----------|-----------|-----------|------------|
| 5 | 7½ | 1.1 | 0.8 (0.4) | 0.1 | 0.2 |
| 1 | 7½ | 0.6 | 0.6 (0.4) | 0.09 | 0.4 (0.45) |
| 0.2 ²⁹ | 6½ | 2 (17) | 2 (10) | 0.2 (1.5) | 0.8 (6.3) |
| 0.2 | 6½ | 2 (17) | 2 (14) | 0.3 (1.6) | 0.8 (6.4) |
| 0.06 | 5½ | 5 (29) | 6 (32) | 0.4 (3.7) | 2 (12) |
| 0.006 | 4½ | 25 (114) | 21 (119) | 3 (21) | 9 (50) |
| 0.0005 | 3½ | 103 (517) | 109 (536) | 56 (219) | 55 (283) |

NOTES

27. Open circuit voltage is typical, measured from input HI to LO, SHI and SLO open. For 1 Ω to 1 MΩ ranges using an external digital multimeter (DMM) set to 10 MΩ input impedance; for 10 MΩ to 1 GΩ ranges, set external DMM to >10 GΩ input impedance.

28. Noise values are based on 1000 readings with autozero on and using low thermal 4-wire short. RMS noise is typical. Additional peak noise is guaranteed.

29. With line sync on.

Resistance Characteristics

Maximum 4-Wire Ohms Lead Resistance

5 Ω per lead for 1 Ω range, 10% of range per lead for 10 Ω to 1 k Ω ranges; 1 k Ω per lead for all other ranges.

Offset Compensation

Selectable on 4-wire, 1 Ω to 100 k Ω ranges.

Open Lead Detector

Default is off.

Autozero Off Error

For 2-wire ohms, ± 1 $^{\circ}\text{C}$ and ≤ 10 minutes, add $\pm(8$ ppm of reading) + 1.5 m Ω for 10 Ω range, 15 m Ω for 100 Ω and 1 k Ω ranges, 150 m Ω for 10 k Ω range, 1.5 Ω for 100 k Ω range, and 15 Ω for all other ranges. For 4-wire ohms, ± 1 $^{\circ}\text{C}$ and ≤ 10 minutes, add $\pm(8$ ppm of reading).

Input Current Limit

For signals with a magnitude of +12 V to +40 V or -12 V to -40 V: ± 13 mA source or sink, typical. For signals with a magnitude of greater than +40 V or -40 V: ± 130 μA source or sink, typical.

DC Current

Enhanced Accuracy (within 30 days of autocalibration, $T_{\text{OPER}} \pm 5$ $^{\circ}\text{C}$ from T_{ACAL})

| Range ³⁰ | Resolution | Maximum Burden Voltage | Accuracy \pm (ppm of reading + ppm of range) | | | | |
|--------------------------|-----------------|------------------------|---|--|--|--|---------------------------------------|
| | | | 24 Hour $T_{\text{CAL}} \pm 1$ $^{\circ}\text{C}$ ³¹ | 90 Day $T_{\text{CAL}} \pm 5$ $^{\circ}\text{C}$ | 1 Year $T_{\text{CAL}} \pm 5$ $^{\circ}\text{C}$ | 2 Year $T_{\text{CAL}} \pm 5$ $^{\circ}\text{C}$ | Temperature Coefficient ³² |
| 10.000000 μA | 1 pA | 15 mV | 30 + 30 | 75 + 30 | 75 + 30 | 75 + 30 | 0.15 + 0.1 |
| 100.000000 μA | 10 pA | 15 mV | 20 + 5 | 60 + 9 | 60 + 9 | 60 + 9 | 0.15 + 0.1 |
| 1.00000000 mA | 100 pA | 15 mV | 30 + 5 | 60 + 9 | 60 + 9 | 60 + 9 | 0.15 + 0.1 |
| 10.0000000 mA | 1 nA | 20 mV | 40 + 5 | 60 + 9 | 60 + 9 | 60 + 9 | 0.15 + 0.1 |
| 100.000000 mA | 10 nA | 200 mV | 50 + 18 | 150 + 30 | 150 + 30 | 150 + 30 | 0.15 + 0.1 |
| 1.00000000 A | 100 nA | 400 mV | 150 + 50 | 400 + 50 | 400 + 50 | 400 + 50 | 0.15 + 0.1 |
| 3.0000000 A | 1 μA | 1300 mV | 200 + 40 | 400 + 40 | 400 + 40 | 400 + 40 | 0.15 + 0.1 |

Accuracy

| Range ³⁰ | Resolution | Maximum Burden Voltage | Accuracy \pm (ppm of reading + ppm of range) | | | | |
|--------------------------|-----------------|------------------------|---|--|--|--|---------------------------------------|
| | | | 24 Hour $T_{\text{CAL}} \pm 1$ $^{\circ}\text{C}$ ³¹ | 90 Day $T_{\text{CAL}} \pm 5$ $^{\circ}\text{C}$ | 1 Year $T_{\text{CAL}} \pm 5$ $^{\circ}\text{C}$ | 2 Year $T_{\text{CAL}} \pm 5$ $^{\circ}\text{C}$ | Temperature Coefficient ³² |
| 10.0000000 μA | 1 pA | 15 mV | 30 + 30 | 100 + 30 | 125 + 40 | 175 + 50 | 10 + 8 |
| 100.000000 μA | 10 pA | 15 mV | 20 + 5 | 75 + 12 | 100 + 15 | 150 + 20 | 10 + 3 |
| 1.00000000 mA | 100 pA | 15 mV | 30 + 5 | 75 + 12 | 100 + 15 | 150 + 20 | 10 + 3 |
| 10.0000000 mA | 1 nA | 20 mV | 40 + 5 | 75 + 12 | 100 + 15 | 150 + 20 | 10 + 3 |
| 100.000000 mA | 10 nA | 200 mV | 50 + 18 | 300 + 30 | 400 + 30 | 500 + 30 | 50 + 5 |
| 1.00000000 A | 100 nA | 400 mV | 150 + 50 | 400 + 50 | 450 + 50 | 500 + 50 | 10 + 10 |
| 3.0000000 A | 1 μA | 1300 mV | 200 + 40 | 400 + 40 | 450 + 40 | 500 + 40 | 10 + 10 |

NOTES

30. 20% overrange supported for all ranges except for 3 A, which is 1% supported.

31. Relative to calibration accuracy.

32. Add per degree from $T_{\text{CAL}} \pm 5$ $^{\circ}\text{C}$.

RMS Noise (additional peak noise uncertainty)³³

Applies to ± ppm of range.

Peak noise uncertainty is included in DC specifications for ≥1 PLC.

Add peak noise uncertainty to measurements when <1 PLC.

Examples

1 mA at 0.006 PLC: 9 (from Accuracy table) + 20 (additional peak noise uncertainty) = 29 ppm of range.

1 mA at 1 PLC: 9 + 0 = 9 ppm of range.

| NPLC | Digits | 10 µA | 100 µA | 1 mA | 10 mA | 100 mA | 1A | 3A |
|-------------------|--------|------------|----------|-----------|-----------|-----------|----------|-----------|
| 5 | 7½ | 0.15 | 0.14 | 0.09 | 0.1 | 0.3 | 0.3 | 0.2 |
| 1 | 7½ | 0.4 | 0.13 | 0.1 | 0.1 | 0.5 | 0.5 | 0.3 |
| 0.2 | 6½ | 0 (220) | 0 (23) | 0.2 (3.4) | 0.2 (1.6) | 2 (10) | 2 (11) | 0.7 (4.6) |
| 0.2 ³⁴ | 6½ | 120 (260) | 12 (26) | 1.2 (3.8) | 0.3 (1.8) | 1.9 (9.8) | 2 (10) | 0.8 (5) |
| 0.06 | 5½ | 130 (280) | 12 (29) | 1.3 (5.6) | 0.4 (3.9) | 2 (14) | 2 (14) | 1.2 (7.7) |
| 0.006 | 4½ | 130 (350) | 14 (42) | 3 (20) | 2 (20) | 4 (30) | 4 (31) | 7 (51) |
| 0.0005 | 3½ | 260 (2110) | 30 (300) | 20 (150) | 20 (160) | 30 (190) | 30 (190) | 70 (510) |

DC Current Characteristics

| Range | 10 µA | 100 µA | 1 mA | 10 mA | 100 mA | 1 A | 3 A |
|---|--------|--------|-------|--------|--------|--------|--------|
| Effective Internal Shunt Value³⁵ | 1 kΩ | 100 Ω | 10 Ω | 1 Ω | 0.1 Ω | 0.1 Ω | 0.1 Ω |
| Autozero Off Error: For ±1 °C and ≤10 minutes add ±(8 ppm of reading + range error) | 150 pA | 1.5 nA | 15 nA | 150 nA | 15 µA | 150 µA | 150 µA |
| Overload Recovery: For each additional sustained amp beyond ±1.5 A, add the following initial ppm of range error until thermally settled after overload recovery | 15500 | 1800 | 150 | 150 | 6500 | 200 | — |

Temperature

4-Wire RTD or 3-Wire RTD

Types: 100 Ω platinum PT100, D100, F100, PT385, PT3916; or user-configurable 0 Ω to 10 kΩ.

| Type | Range | Resolution | Accuracy ± °C | |
|--------------------------|-----------------|------------|--------------------------------|---------------------------------------|
| | | | 2 Year, T _{CAL} ±5 °C | Temperature Coefficient ³⁶ |
| 4-Wire RTD | -200° to 400 °C | 0.01 °C | 0.09 °C | 0.003 °C/ °C |
| 3-Wire RTD ³⁷ | -200° to 400 °C | 0.01 °C | 0.75 °C | 0.003 °C/ °C |

Thermistor

Types: 2.252 kΩ, 5 kΩ, and 10 kΩ.

| Type | Range | Resolution | Accuracy ± °C | |
|------------|-----------------|------------|--------------------------------|---------------------------------------|
| | | | 2 Year, T _{CAL} ±5 °C | Temperature Coefficient ³⁶ |
| Thermistor | -80° to +150 °C | 0.01 °C | 0.08 °C | 0.002 °C/ °C |

NOTES

33. Noise values are based on 1000 readings with autozero on and AMPS terminal open. RMS noise is typical. Additional peak noise is guaranteed.
 34. With line sync on.
 35. Values are typical and guaranteed by design.
 36. Add per degree from T_{CAL} ±5 °C; specifications without autocalibration.
 37. For 3-wire RTD, accuracy is for < 0.1 Ω lead resistance mismatch for input HI and LO. Add 0.25 °C/ 0.1 Ω of HI-LO lead resistance mismatch.

Thermocouple

Types: B, E, J, K, N, R, S, T

| Type | Range | Resolution | Accuracy ± °C | |
|------|------------------|------------|--|---------------------------------------|
| | | | 2 Year, T _{CAL} ±5 °C ³⁸ Simulated Reference Junction | Temperature Coefficient ³⁶ |
| B | 350 to +1820 °C | 0.1 °C | 0.9 °C | 0.03 °C/ °C |
| E | -200 to +1000 °C | 0.001 °C | 0.4 °C | 0.03 °C/ °C |
| J | -200 to +760 °C | 0.001 °C | 0.4 °C | 0.03 °C/ °C |
| K | -200 to +1372 °C | 0.001 °C | 0.4 °C | 0.03 °C/ °C |
| N | -200 to +1300 °C | 0.001 °C | 0.4 °C | 0.03 °C/ °C |
| R | 0 to +1768 °C | 0.1 °C | 0.9 °C | 0.03 °C/ °C |
| S | 0 to +1768 °C | 0.1 °C | 0.9 °C | 0.03 °C/ °C |
| T | -100 to +400 °C | 0.001 °C | 0.4 °C | 0.03 °C/ °C |

Continuity

| Range ³⁹ | Resolution | Test Current | Open Circuit Voltage | Accuracy ±(ppm of reading + ppm of range) | |
|---------------------|------------|--------------|----------------------|---|---------------------------------------|
| | | | | 2 Year, T _{CAL} ±5 °C | Temperature Coefficient ⁴⁰ |
| 1.0000 kΩ | 100 mΩ | 1 mA | 14.0 V | 100 + 100 | 2.5 + 1 |

Continuity Characteristics

Continuity High Limit User-selectable; default 10 Ω.

NOTES

38. Exclusive of cold-junction errors.

39. Specifications exclude lead resistance.


40. Add per degree from T_{CAL} ±5 °C; specifications without autocalibration.

Digitize Voltage

Accuracy (Input Impedance AUTO)

| Range ^{41, 42} | Resolution ⁴³ | Input Impedance ⁴⁴ | Accuracy ±(ppm of reading + ppm of range) | | | |
|-------------------------|--------------------------|-------------------------------|---|----------------------------------|----------------------------------|--|
| | | | 90 Day T _{CAL} ±5 °C | 1 Year T _{CAL} ±5 °C | 2 Year T _{CAL} ±5 °C | Temperature Coefficient ⁴⁵ |
| 100.000 mV | 1 µV | >10 GΩ or 10 MΩ ±1% | 210 + 100 | 220 + 100 | 230 + 100 | 15 + 20 |
| 1.00000 V | 10 µV | >10 GΩ or 10 MΩ ±1% | 110 + 75 | 120 + 75 | 130 + 75 | 15 + 20 |
| 10.0000 V | 0.1 mV | >10 GΩ or 10 MΩ ±1% | 110 + 75 | 120 + 75 | 130 + 75 | 10 + 20 |
| 100.000 V ⁴⁶ | 1 mV | 10 MΩ ±1% | 110 + 75 | 120 + 75 | 130 + 75 | 15 + 20 |
| 1000.00 V ⁴⁷ | 10 mV | 10 MΩ ±1% | 110 + 75 | 120 + 75 | 130 + 75 | 10 + 20 |

DC-Coupled Additional Noise Uncertainty, Typical ⁴⁸

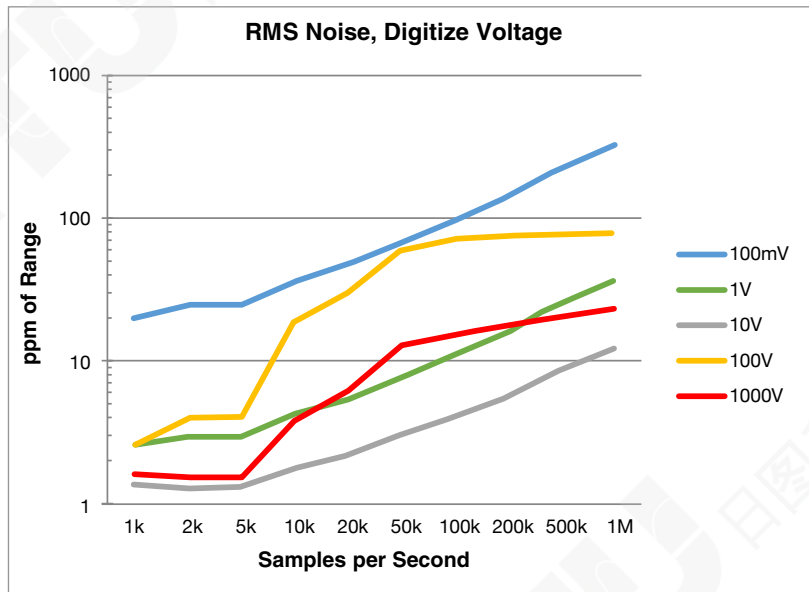

NOTES


41. For DC coupling, 20% overrange for 100 mV to 100 V. For AC coupling, 500% overrange 100 mV to 100 V. 1% for 1000 V range DC coupling.
42. Accuracy with sample rate 1 k per second, aperture auto, and 100 reading buffer average.
43. Power up default is 4½ digits.
44. User-selectable.
45. Add per degree from T_{CAL} ± 5%.
46. For 100 V range, input impedance auto and without ACAL, add 100 ppm of range additional uncertainty and 15 ppm/°C additional uncertainty for "of range" temperature coefficient for operation outside of T_{CAL} ± 5 °C.
47. For signal levels greater than 500 V, add 0.02 ppm/V to the ppm of the readings specification for measurements exceeding 500 V.
48. Specified with aperture Auto and 4-wire short on input terminals. For 100 V range, input impedance 10 MΩ, multiply by 2.5. For all ranges and sample rate > 1 k, add an additional 3× RMS noise uncertainty to ppm of range.

Digitize Current

DC Accuracy ⁴⁹

| Range ⁵⁰ | Resolution ⁵¹ | Burden Voltage | Accuracy ± (ppm of reading + ppm of range) | | | |
|---------------------|--------------------------|----------------|--|----------------------------------|----------------------------------|--|
| | | | 90 Day T _{CAL} ±5 °C | 1 Year T _{CAL} ±5 °C | 2 Year T _{CAL} ±5 °C | Temperature Coefficient ⁵² |
| 10.0000 µA | 0.1 nA | 15 mV | 150 + 75 | 160 + 75 | 170 + 75 | 30 + 15 |
| 100.000 µA | 1 nA | 15 mV | 150 + 75 | 160 + 75 | 170 + 75 | 30 + 15 |
| 1.00000 mA | 10 nA | 15 mV | 150 + 75 | 160 + 75 | 170 + 75 | 30 + 15 |
| 10.0000 mA | 100 nA | 20 mV | 150 + 75 | 160 + 75 | 170 + 75 | 30 + 15 |
| 100.000 mA | 1 µA | 200 mV | 340 + 100 | 450 + 100 | 560 + 100 | 50 + 20 |
| 1.00000 A | 10 µA | 400 mV | 400 + 110 | 500 + 110 | 600 + 110 | 50 + 25 |
| 3.00000 A | 100 µA | 1300 mV | 650 + 150 | 900 + 150 | 900 + 150 | 50 + 25 |

Additional Noise Uncertainty, Typical ⁵³

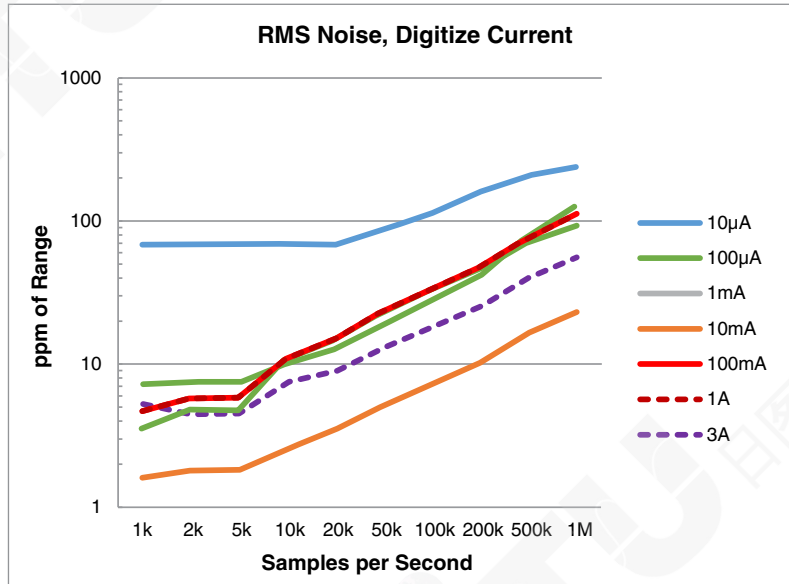

NOTES

49. Accuracy with sample rate 1 k per second, aperture auto, and 100 reading buffer average.

50. 20% overrange on all ranges except 3.3% for 3 A range.

51. Power up default is 4½ digits.

52. Add per degree from T_{CAL} ±5 °C.

53. Specified with aperture Auto and open input terminals. For all ranges and for ≥1 k sample rate, add an additional 3× RMS noise uncertainty to ppm of range.

Digitizer Characteristics

| | |
|--|--|
| Maximum Resolution | 18 bits. |
| Measurement Input Coupling | DC or AC (voltage only). |
| Sampling Rate ⁵⁴ | Programmable 1 k through 1 million. |
| Volatile Sample Memory with Timestamp | 27.5 million. |
| Minimum Record Time | 1 µs. |
| Timestamp Resolution | 1 ns with standard or full buffer style. 1 µs with compact buffer style. |
| Timestamp Accuracy | With standard or full buffer style, 20 ns between adjacent readings, with total buffer time <2 s. With compact buffer style, 2 µs adjacent readings, with total buffer time <2 s. |
| Maximum Record Length | 8 million. |

Typical Reading Rates, 60 Hz (50 Hz) Operation^{55, 56, 57, 58}

| NPLC | Digits | Functions: DC Voltage (10 V), 2-wire Ohms (≤10 kΩ), DC Current (1 mA) | | Functions: 4-wire ohms (≤1 kΩ), 4-wire/3-wire RTD | | Functions: Thermistor | | Functions: Dry Circuit (≤1 kΩ) | |
|--------|--------|--|-------------------------------|---|-------------------------------|-----------------------------|-------------------------------|-----------------------------------|-------------------------------|
| | | Measurements Into Buffer | Measurements Into Computer | Measurements Into Buffer | Measurements Into Computer | Measurements Into Buffer | Measurements Into Computer | Measurements Into Buffer | Measurements Into Computer |
| 1 | 7½ | 59.8 (49.8) | 58 (48) | 29 (24) | 28 (24) | 57 (48) | 57 (48) | 27 (23) | 26 (22) |
| 0.2 | 6½ | 295 (240) | 250 (210) | 128 (109) | 119 (100) | 230 (200) | 230 (200) | 100 (89) | 96 (85) |
| 0.06 | 5½ | 965 (810) | 950 (800) | 310 (280) | 315 (280) | 900 (750) | 900 (750) | 190 (180) | 190 (180) |
| 0.006 | 4½ | 7500 (6700) | 7300 (6500) | 750 (730) | 740 (720) | 6800 (6000) | 6800 (6000) | 295 (290) | 295 (290) |
| 0.0005 | 3½ | 26000 (26000) | 24000 (24000) | 860 (860) | 860 (860) | 18000 (18000) | 18000 (18000) | 310 (310) | 310 (310) |

Digitize, Typical

| Sampling Rate | Digits | Resolution | Measurements Into Computer ⁵⁸ |
|---------------|--------|------------|--|
| 10 kS/s | 5½ | 18 | 9700 |
| 20 kS/s | 4½ | 16 | 19000 |
| 50 kS/s | 4½ | 16 | 44400 |
| 100 kS/s | 4½ | 15 | 80000 |
| 1 MS/s | 3½ | 12 | 108000 |

NOTES

54. Sample rate is not continuously adjustable. For valid discrete settings, see the DMM7512 Reference Manual.

55. Reading speeds for autozero off, fixed range, autodelay off. Offset compensation off and open lead detector off where applicable.

56. Buffer measurements: For <0.2 PLC, multisample, single buffer transfer binary reading only.

57. PC measurements: For 1 and 0.2 PLC single reading and single transfer to computer (USB).

58. Reading rates using factory default operating conditions and autorange off, autodelay off. Speeds include measurement and data transfer out of the USB. ≥1000 readings with binary transfer over USB.

System Performance, Typical

Mode 3½-digit, autozero off, 0.0005 PLC, excludes measurement time.

Time includes function change from DC voltage or 2-wire ohms to listed function.

| Function | Function Change (ms) | Range Change (ms) |
|------------------------------------|----------------------|-------------------|
| DC Voltage or 2-wire ohms (<10 kΩ) | 6 | 1.3 |
| 4-wire ohms (<10 kΩ) | 7 | 1.3 |
| DC Current | 7 | 1.3 |
| Digitize Voltage or Current | 7 | 1.3 |

Ranges for Function Change Times

Function change times apply to the ranges listed in the table below.

| Function | Range |
|-----------------------|-----------------------|
| DC Voltage | 10 V |
| 2-wire or 4-wire Ohms | 1 kΩ |
| DC Current | 1 mA |
| Thermocouple | Use DC Voltage rates |
| Thermistor | Use 2-wire Ohms rates |

| Buffer Transfer Speed (Binary) | Measurements into Computer (per second) | |
|--|---|--------|
| | USB | LAN |
| Average for 1000 readings | 280000 | 270000 |
| Average for 1000 readings with timestamp | 170000 | 140000 |

Triggering

Time Base Accuracy 25 ppm.

Trigger Source Analog DCV, DCI, or any system trigger.

Trigger Coupling DC.

Input Trigger Latency^{59, 60, 61} <225 ns.

Input Trigger Jitter^{59, 60} <50 ns.

Sample period Jitter^{59, 60} <1 ns.

DMM Triggers

EXT TRIG IN and OUT 0 V to 5 V logic signal input and output, TTL compatible.

EXT trigger latency (IN and OUT) <400 ns.

EXT trigger latency (IN or OUT) <200 ns (guaranteed by design).

NOTES

59. Guaranteed by design; for digital I/O only.

60. Stimulus command required to meet specifications.

61. If using trigger model, add 200 ns uncertainty.

Analog Triggering ⁶²

Analog Level, Edge, or Window Trigger Types ⁶³

| Trigger Characteristics | Voltage Input | Current Input |
|---|------------------|-------------------|
| Input Range | 100 mV to 1000 V | 10 μ A to 3 A |
| Resolution | 0.05% | 0.05% |
| Basic Accuracy ($T_{ACAL} \pm 5$ °C) ^{64, 65} | 1% | 1% |

Analog Trigger Latencies

| | Digital I/O | External |
|----------------|-----------------------|-----------------------|
| Positive Logic | 800 ns + 40 ns jitter | 930 ns + 40 ns jitter |
| Negative Logic | 800 ns + 40 ns jitter | 840 ns + 40 ns jitter |

Window Filter and Memory (buffer)

| | |
|---|--|
| Window Filter Size | 0 to 10% of reading, where 0 averages all readings. |
| Memory | Up to 27.5 million timestamped readings with the compact buffer style, with additional memory available using an external USB flash drive. |
| Maximum Internal Memory (Buffer) | 27.5 million readings with the compact buffer style (6½-digit without formatting), 11 million readings with the standard or full buffer style. |

NOTES

62. For DC coupled, the trigger level can be set up to 100% of measure range.

63. Rising or falling edge triggering supported. Window trigger requires setting two independent levels.

64. Trigger event occurs after the threshold crossing at a time determined by total trigger latencies.


65. Accuracy specifications require user ACAL and are verified with level trigger amplitude set to 50% of range with a 100 Hz sine wave at 100% full scale of range. High frequency rejection is off. NPLC 0.0005 (DC voltage/DC current) or aperture 1 μ s for digitize voltage or digitize current. Specified for fixed range, autozero off. For DC current and digitized DC current 3 A range, add an additional 2%.

General Instrument Specifications

| | |
|---|--|
| Input Protection | 1010 V DC all ranges and functions on HI and LO terminals; 350 V all ranges and functions on sense HI, sense LO terminals; 250 V rated current input terminal; fused 3 A range; current input terminals protected to 1 kV. |
| 3 A Input Fuse Protection | 3.5 A, 1 kV fast blow type; Keithley part number DMM7510-FUSE-3A. |
| Common Mode Isolation | 500 VDC or ACV_{PEAK} LO to chassis. All terminals $>10\ \Omega$, $<350\ \text{pF}$ any terminal to chassis. |
| Power Line | Universal input, 100 V to 240 V. |
| Line Frequency | 50 Hz or 60 Hz, automatically sensed at power-up. |
| Power Consumption | 165 VA. |
| Operating Environment | Specified for 0 °C to 50 °C, $\leq 70\%$ relative humidity up to at 35 °C; derate 3% relative humidity per °C, 35 °C to 50 °C. |
| Storage Environment | -25 °C to 65 °C. |
| Altitude | Maximum 2000 m (6562 ft) above sea level. |
| Pollution Degree | 2. |
| Real Time Clock | Lithium battery backup (3+ years battery life). |
| EMC | Conforms to European Union EMC Directive. |
| Safety | NRTL listed to UL61010-1 and CSA C22.2 No 61010-1; conforms with European Union Low Voltage Directive. |
| Vibration | MIL-PRF-28800F Class 3, Random. |
| Warm-up | 4 hours to rated accuracy. |
| Input Signal Connections | Rear safety banana jacks. |
| Cooling | Forced air, side intake, and rear exhaust. |
| Dimensions | Rack Mount: 44 mm high \times 483 mm wide \times 696 mm deep (1.7 in. \times 19 in. \times 27.41 in.) |
| Shipping Weight | 11.3 kg (25.0 lb.). |
| Digital I/O | |
| Connector | 9-pin female D. |
| 5V Power Supply Pin | Limited to 500 mA at $>4\ \text{V}$ (solidstate fuse protected). |
| Lines | Six input/output, user-defined, for digital I/O or triggering. |
| Input Signal Levels: | 0.7 V (maximum logic low) 3.7 V (minimum logic high). |
| Input Voltage Limits: | -0.25 V (absolute minimum) +5.25 V (absolute maximum). |
| Maximum Source Current | +2.0 mA at $>2.7\ \text{V}$ (per pin). |
| Maximum Sink Current | -50 mA at 0.7 V (per pin, solid-state fuse protected). |
| Handler | User-defined start of test, end of test, four category bits |
| Math Functions | Rel, dB, Limit Test, Percentage, $1/x$, and $mX + b$. |
| Remote Interface | |
| LAN | RJ-45 connector, 10/100BT; Virtual Front Panel. |
| USB Device (front panel, type B) | 2.0 full speed, USBTMC compliant. |
| USB Host (front panel, type A) | USB 2.0, support for flash drives, FAT 32. |
| LXI Compliance | LXI version 1.4 Core 2011. |

Language Embedded Test Script Processor (TSP) accessible from any host interface; responds to high-speed test scripts comprised of remote commands and statements (for example, branching, looping, math); able to execute high-speed test scripts stored in memory without host intervention; also SCPI (default command set).

Expansion Interface The TSP-Link expansion interface allows TSP-enabled instruments to trigger and communicate with each other. See the figure below.

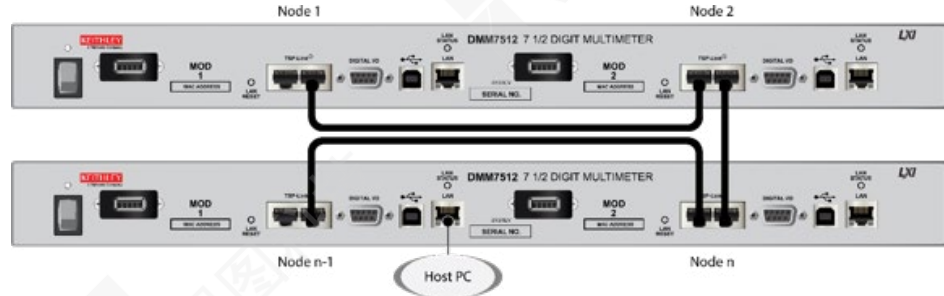

The DMM7512 has four TSP-Link connectors (two on each module) to make it easier to connect instruments in a sequence.

- Once instruments are interconnected through the TSP-Link expansion interface, a computer can access all of the resources of each source measure instrument through the host interface of any TSP-Link instrument.
- A maximum of 32 TSP-Link nodes can be interconnected. Each source-measure module uses one TSP-Link node.

IP configuration Static or DHCP (manual or automatic).

Ordering Information

DMM7512 Dual Channel 7 ½-Digit Sampling Multimeter

Supplied Accessories

| | |
|-------------|---|
| 012178100 | Test Lead Kit, Quantity 4 |
| CA-18-16A | LAN Crossover Cable, 40 cm (16 in), quantity 2 |
| 174710700 | Shielded Crossover Cable with RJ-45 Connector, 1.5 m (5 ft), quantity 1 |
| CA-568-120A | Green and Yellow Ground Cable, 3.0 m (120 in), quantity 1 |
| 4299-13 | 1U High Fixed Rack Mount Kit, quantity 1 |
| 0713411 | Safety Precautions Document |
| 071357600 | DMM7512 7½-Digit Multimeter Instrument Information |

Instruction Manuals/Documentation (available at www.rituchina.com/DMM7512)

DMM7510 7.5 Digit Graphical Sampling Multimeter Reference Manual

DMM7510 7.5 Digit Graphical Sampling Multimeter User's Manual

Software and Drivers (available at www.rituchina.com)

IVI/VISA Drivers for Microsoft® Visual Basic®, Visual C/C++®

Keithley Test Script Builder available at <https://www.rituchina.com/keithley-test-script-builder>

Power Cord Options

| | |
|-----|-------------------------------|
| A0 | North America (120 V, 60 Hz) |
| A1 | Universal Euro (220 V, 50 Hz) |
| A2 | United Kingdom (240 V, 50 Hz) |
| A3 | Australia (240 V, 50 Hz) |
| A4 | Chile, Italy (220 V, 50 Hz) |
| A5 | Switzerland (220 V, 50 Hz) |
| A6 | Japan (100 V, 50/60 Hz) |
| A7 | Denmark (230 V, 50 Hz) |
| A8 | Israel (230 V, 50 Hz) |
| A9 | Argentina (220 V, 50 Hz) |
| A10 | China (230 V, 50 Hz) |
| A11 | India (230 V, 50 Hz) |
| A12 | Brazil (127 V/220 V, 60 Hz) |
| A99 | No power cord |

Available Accessories

Test Leads and Probes

| | |
|------|--|
| 1751 | Safety Test Leads |
| 1754 | 2-Wire Universal 10-Piece Test Lead Kit |
| 1756 | General Purpose Test Lead Kit |
| 5804 | Kelvin (4-Wire) Universal 10-Piece Test Lead Kit |
| 5805 | Kelvin (4-Wire) Spring-Loaded Probes |
| 5806 | Kelvin Clip Lead Set |
| 5808 | Low Cost Single-pin Kelvin Probe Set |
| 5809 | Low Cost Kelvin Clip Lead Set |
| 8606 | High Performance Modular Probe Kit |
| 8610 | Low Thermal Shorting Plug |

Replacement Fuses

| | |
|-----------------|---|
| FU-106-3.15 | Line Power Fuse, 250 V, 3.15 A, Slow Blow 5 × 20 mm |
| DMM7510-FUSE-3A | 3.5 A Current Fuse |

Cables, Connectors, Adapters

| | |
|---------|---|
| CA-18-1 | Shielded Dual Banana Cable, 1.2 m (4 ft.) |
|---------|---|

Cables

| | |
|-----------|--|
| CA-180-3A | CAT5 Crossover Cable for TSP-Link / Ethernet |
| USB-B-1 | USB Cable, Type A to Type B, 1 m (3.3 ft) |

Triggering and Control

| | |
|------------|---|
| 2450-TLINK | DB-9 to Trigger Link Connector Adapter |
| 8501-1 | Trigger Link Cable, DIN-to-DIN, 1 m (3.2 ft.) |
| 8501-2 | Trigger Link Cable, DIN-to-DIN, 2 m (6.5 ft.) |
| 8503 | DIN-to-BNC Trigger Cable |

Rack Mount Kit

| | |
|---------|------------------------------|
| 4299-13 | 1U High Fixed Rack Mount Kit |
|---------|------------------------------|

Available Services

Extended Warranties

| | |
|---------------|---|
| DMM7512-EW | 1 Year Factory Warranty Extended to 2 Years from Date of Shipment |
| DMM7512-3Y-EW | 1 Year Factory Warranty Extended to 3 Years from Date of Shipment |
| DMM7512-5Y-EW | 1 Year Factory Warranty Extended to 5 Years from Date of Shipment |

Calibration Contracts

| | |
|--------------------|--|
| C/DMM7512-3Y-STD | KeithleyCare 3 Year Std Calibration Plan |
| C/DMM7512-3Y-DATA | KeithleyCare 3 Year Calibration w/Data Plan |
| C/DMM7512-3Y-17025 | KeithleyCare 3 Year ISO-17025 Calibration Plan |
| C/DMM7512-5Y-STD | KeithleyCare 5 Year Std Calibration Plan |
| C/DMM7512-5Y-DATA | KeithleyCare 5 Year Calibration w/Data Plan |
| C/DMM7512-5Y-17025 | KeithleyCare 5 Year ISO-17025 Calibration Plan |

Warranty Information

| | |
|--------------------------|--|
| Warranty Summary | This section summarizes the warranties of the DMM7512. For complete warranty information, refer to the DMM7512 Reference Manual. Any portion of the product that is not manufactured by Keithley is not covered by this warranty and Keithley will have no duty to enforce any other manufacturer's warranties. |
| Hardware Warranty | Keithley Instruments, Inc. warrants the Keithley manufactured portion of the hardware for a period of one year from defects in materials or workmanship; provided that such defect has not been caused by use of the Keithley hardware which is not in accordance with the hardware instructions. The warranty does not apply upon any modification of Keithley hardware made by the customer or operation of the hardware outside the environmental specifications. |
| Software Warranty | Keithley warrants for the Keithley produced portion of the software or firmware will conform in all material respects with the published specifications for a period of ninety (90) days; provided the software is used on the product for which it is intended in accordance with the software instructions. Keithley does not warrant that operation of the software will be uninterrupted or error-free, or that the software will be adequate for the customer's intended application. The warranty does not apply upon any modification of the software made by the customer. |



日图抖音号



日图公众号

深圳总部

深圳市南山区留仙大道南山云谷创新产业园二期 6 栋一楼东座
电话：0755-83680722(8 线)

上海分公司

上海市闵行区中春路 8633 弄万科七宝国际 26 幢 701 室
电话：021-33888891/3/5
手机：13564654980

广州分公司

广州市科学城科学大道中 97 号科汇金谷 J 栋东座 808 室
电话：020-31604020
手机：18027340836

西安分公司

陕西省西安市雁塔区长安中路南飞鸿广场 3 号楼 1813 室
手机：15529365365

杭州分公司

浙江省杭州市萧山区盈丰街道鸿宁路 1819 号左右世界 1 幢 1 单元 702-3
电话：0571-86856181
手机：18668225058

重庆分公司

重庆市观音桥茂业东方时代大厦 35 楼 3509 室
电话：023-67904187
手机：13896060852

苏州分公司

苏州苏州工业园区科营路 2 号中新生态大厦 10 楼 1010 室
电话：0512-62515781、0512-62515784
手机：15895400640

香港分公司

香港新界元朗屏厦厦村厦村路 DD125 段 1215-1217lot
电话：+852-24932683

深圳市日图科技有限公司

SHENZHEN RITU SCIENCE TECHNOLOGY CO.,LTD

🌐 www.rituchina.com

☎ 400-616-5217

📍 广东省深圳市南山区留仙大道南山云谷创新产业园二期 6 栋一楼东座

① 如需所有最新配套资料，请立即与日图科技各地分公司联系。